



Posterior Thigh Isometric Force Measurement with Extended Knee

Darío Santos^{1,2,3,4}, Isabel Morales¹, Andrea Mattiozzi⁵, Arleth Peláez⁴,
Sabrina Pérez⁴, Agustín Fernández⁶, Matías Vignoli⁷, Jorge Domínguez⁶,
Mario Battistin⁴, Rodrigo Barboza⁶, Camilo Martínez⁷, Lucia Stefanelli⁷,
Sofía González⁵ and Franco Simini^{1*}

¹Núcleo de Ingeniería Biomédica (NIB), Universidad de la República, Montevideo, Uruguay.

²Department of Rehabilitation, Hospital de Clínicas, Universidad de la República Montevideo, Uruguay.

³British Hospital, Montevideo, Uruguay.

⁴Escuela Universitaria de Tecnología Médica (EUTM), Universidad de la República, Montevideo, Uruguay.

⁵Department of Sports Medicine, Hospital de Clínicas, Montevideo, Uruguay.

⁶MOVI Ltda., Montevideo, Uruguay.

⁷Instituto Superior de Educación Física, Universidad de la República, Montevideo, Uruguay.

Authors' contributions

This work was carried out in collaboration among all authors. Authors DS, IM, SP, LS, SG and FS gave conception and design of the study. Authors DS, IM, AM, LS and FS drafting the article and carried out its critical revision. All authors except authors IM and FS collected the data for research work. Authors DS, IM, AM, AP, AF, JD and FS performed the data analysis and interpretation. All authors read and approved the final manuscript.

Article Information

DOI: 10.9734/JSRR/2019/v23i630141

Editor(s):

(1) Dr. Karl Kingsley, University of Nevada, Las Vegas - School of Dental Medicine, USA.

Reviewers:

(1) Preksha Barot, GMERS Medical College, India.

(2) Vinay Jagga, Prem Physiotherapy and Rehabilitation College, India.

Complete Peer review History: <http://www.sdiarticle3.com/review-history/49921>

Original Research Article

Received 29 April 2019

Accepted 02 July 2019

Published 12 July 2019

ABSTRACT

Aims: The establishment of normal values for the hamstring flexibility and isometric posterior thigh force of healthy adults performing standard motor task consisting of acting against a rubber band in the supine position.

*Corresponding author: E-mail: simini@fing.edu.uy;

Study Design: Observation and ecological.

Place and Duration of Study: During a Sports Medicine three days event (Congreso DePunta) in Uruguay, September 2018.

Methodology: Random samples of 21 men and 16 women practicing different sport activities were asked to have their biomechanics properties measured by DINABANG, which is a novel clinical instrument to guide lower limb rehabilitation. DINABANG measures the force signal during the following specific motor task: in supine position, consists of hip flexion with fully extended knee and with malleolus attached to a rubber band held by the Physical Therapist behind the head of the person, until further effort would lift the person from the mat.

Results: Normal values for body weight specific peak force during isometric effort with extended limb in supine position and malleolus strap tied to an elastic band are (mean \pm SD) $1.7 \pm 0.4 / 1.9 \pm 0.5 \text{ N}\cdot\text{Kg}^{-1}$ for men and $2.1 \pm 0.5 / 2.3 \pm 0.5 \text{ N}\cdot\text{Kg}^{-1}$ for women and weak/strong limb respectively. The volunteer-defined flexibility angles of the healthy young populations (21 men and 16 women) were found to be $67.5^\circ \pm 6.5^\circ$ and $77.5^\circ \pm 9.7^\circ$ merging the distributions of both lower limbs, strong and weak.

Conclusion: These values will be included in subsequent versions of DINABANG to be used in clinical practice to help avoiding muscle strains by quantifying efforts during rehabilitation under Physical Therapist monitoring. DINABANG allows to safely perform a motor task in the medical office. It can be said that DINABANG is compatible with an ecological approach to rehabilitation.

Keywords: Biomechanics; DINABANG; hamstring; knee; normal values; physical therapy; rehabilitation.

1. INTRODUCTION

Lower limb movement analysis has been addressed in several studies to determine the sequence of contraction of posterior and anterior muscles of the thigh [1]. Moreover, muscle force characterization is increasingly important in rehabilitation and sports medicine [2], especially for elite athletes [3,4]. Hamstring injuries occur during sports when the athlete, during terminal swing phase of running [5], extends the lower limb beyond limits. Rehabilitation is very important after injuries or surgical repair. Despite the existence of rehabilitation protocols [6] there is no evidence of validated functional protocols that emulate the specific motor task. Moreover, for football players, rehabilitation is seldom complete [7] giving rise to unwanted sequelae. Considering the importance of a good rehabilitation, it is surprising that little has been published on such measurements. One of the reasons for such lack of protocols and of normal measurements maybe the absence on the market of instruments suitable for fieldwork. To foster quantitative evaluation of rehabilitation and to further the efficiency of sports training, we have developed CINARTRO [8] to quantify knee joint movement, CINAR-3D [9] to estimate leg rotation and DINABANG [10] to measure motor task force for hamstring strains avoidance during guided exercise. To this end, DINABANG is able to measure angular velocity, force and

torque to help the Physical Therapist during hamstring rehabilitation exercises.

This report establishes the first set of isometric normal values using DINABANG in healthy adults, as a contribution to physiological knowledge but primarily to be included in subsequent versions of DINABANG as reference values to compare measurements to.



Fig. 1. The physical therapist, located behind the volunteer's head, holds the elastic band attached to the distal portion of tibia

2. MATERIALS AND METHODS

2.1 Participants

A group of young healthy adults practicing different sport activities at a nonprofessional level was asked to be part of the present research. The study was carried out in accordance with the guidelines contained in the Declaration of

Helsinki and all participants signed an informed consent approved by the University Ethics Committee of the Hospital de Clínicas. We studied a population of $n=37$ athletes (men $n=21$, women $n=16$), whose ages, standing heights and body masses were (mean \pm SD) men: 24.6 ± 3.8 years, 174.3 ± 7.4 cm and 72.4 ± 11.6 Kg, women: 26.0 ± 6.7 years, 166.9 ± 4.0 cm and 61.9 ± 7.5 Kg. The sportspersons were evaluated during a Sports Medicine three days event (*Congreso DePunta*) in Uruguay, September 2018. Participants were excluded if they have had hamstring injuries ever or any knee injury history in the 12 months prior to the event.

2.2 Measurements

DINABANG is an original device [10] to record the force, angular velocity and elastic band vector direction which, along with lower limb length and weight, allows monitoring torque and effort during guided exercise. Among other information, DINABANG provides the isometric force measurement as the maximum value of the force signal. The specific motor task analysed by DINABANG consists of thigh posterior muscles contraction under Physical Therapist direction (Fig. 1). The motor task, in supine position, consists of hip flexion with fully extended knee and with malleolus attached to a rubber band held by the Therapist behind the head of the athlete. There is an instant when, despite increasing the effort, the force signal does not increase anymore because the patient or the Therapist let go, since the lumbar region would be otherwise lifted.

2.3 Design and Procedures

The measurement of thigh posterior muscle force is the result of a special setup by which the person is laying down in supine position on a gymnastic mat. DINABANG strap bracelet is successively attached to the tibia, immediately above the malleolus of the strong and later weak limb. The Physical Therapist is located behind the head of the volunteer holding an elastic TheraBand[®] attached to the strap (Fig. 1) and guides the isometric effort, one limb at a time. The position familiarization phase consists of selecting the most comfortable angle for the active limb, around 60° with respect to the horizontal plane (Fig. 2, angle graph). This angle depends on the flexibility of the volunteer and is estimated by the angle signal given by DINABANG (Fig. 2). The leg is pushed towards 0° , extending the hip with fully extended knee. Once in a comfortable position (60°

approximately, time b in Fig. 2), the athlete is asked to increase the strength of his or her effort until the lumbar region is about to be lifted from the mat (point c in Fig. 2). At this point, there is a drastic decrease in the force applied because the athlete stops his or her effort. The peak force reached is measured by selecting the maximum of the signal (point c , Fig. 2), which therefore represents the necessary force to barely lift the body. The relaxing phase of the limb goes from point c to point d in Fig. 2 while maintaining roughly the same 60° position as held in place by the elastic band.

The average of the comfortable hip flexion angles (three trials per athlete) is a measure of hamstring flexibility score for each limb. We therefore used the "passive straight-leg-raise test" [11] to estimate the flexibility angle.

2.4 Statistical Analysis

We performed Kolmogorov-Smirnov and Shapiro-Wilk tests to assess Gaussian distribution within men's and women's data, as well as within strong and weak limbs of both genders. We applied non-paired t-test to men versus women strong limb and weak limb hamstring flexibility angle (bilateral) and hamstring isometric force (unilateral) respectively. Type 1 error was set at 5% and all data were analysed with XLSTAT Free[®].

3. RESULTS

The maximum isometric standardized force measurements ($N \cdot Kg^{-1}$) [12][13] were separated in strong and weak limb series, for men and women as shown in Table 1. For both lower limbs (weak and strong) women body weight-specific force is higher than men's which represents a statistically different physiologic reality (Table 1).

Fig. 3 shows the four adjusted distribution curves of the posterior thigh isometric force of strong and weak lower limbs of a normal population. The mean force exerted is $1.7 \pm 0.4 N \cdot Kg^{-1}$ and $1.9 \pm 0.5 N \cdot Kg^{-1}$ for men and $2.1 \pm 0.5 N \cdot Kg^{-1}$ and $2.3 \pm 0.5 N \cdot Kg^{-1}$ for women, exercising the weak and strong limb respectively. The women curves are displaced towards higher values, with respect to men.

In a similar way, the measurements of the flexibility angle selected by each athlete to perform the isometric effort are given in Table 2. The weak limb flexibility angle distribution

coincides with the strong limb flexibility angle distribution, which allow us to show a single distribution (Table 2): 67.5° for men and 77.5° for women. Women flexibility angle is thus larger by about 10 degrees than the selected angle for men (Table 2).

Fig. 4 shows the adjusted distribution curves of men and women flexibility angle resulting from 42 and 32 lower limbs respectively. The normal population of men selects an angle of 67.5° ± 6.5° while women select an angle of 77.5° ± 10°. The flexibility of women is greater than men's by about 13%.

4. DISCUSSION

We believe that the measurements reported here are the first to be taken by a clinical instrument such as DINABANG. Isometric efforts of the order of 2 N·Kg⁻¹ of body weight are similar to other muscle force measurements such as the isometric mid-thigh pull (IMTP) motor task for which a standardized value of 0.92 ± 0.15 N·Kg⁻¹ [3]. Our Fig of 2.0 ± 0.5 N·Kg⁻¹ is higher than the IMTP because strength developed by the hamstring opposing the elastic band is by far larger than the strength of the downwards mid-thigh pull.

Table 1. Weak/strong standardized peak force analysis of 74 lower limbs

	Weak limb (n=37)		Strong limb (n=37)	
	Mean	SD	Mean	SD
Men	1.7	0.4	1.9	0.5
Women	2.1	0.5	2.3	0.5
p values <	0.01		0.03	

Table 2. Weak/strong and men/women flexibility angle analysis

	Men (n=42)		Women (n=32)	
	Mean	SD	Mean	SD
Angle Strong Limb (°)	67.5	6.6	77.9	10.7
Angle Weak Limb (°)	67.5	6.5	77.1	8.7
p values =	0.96		0.80	

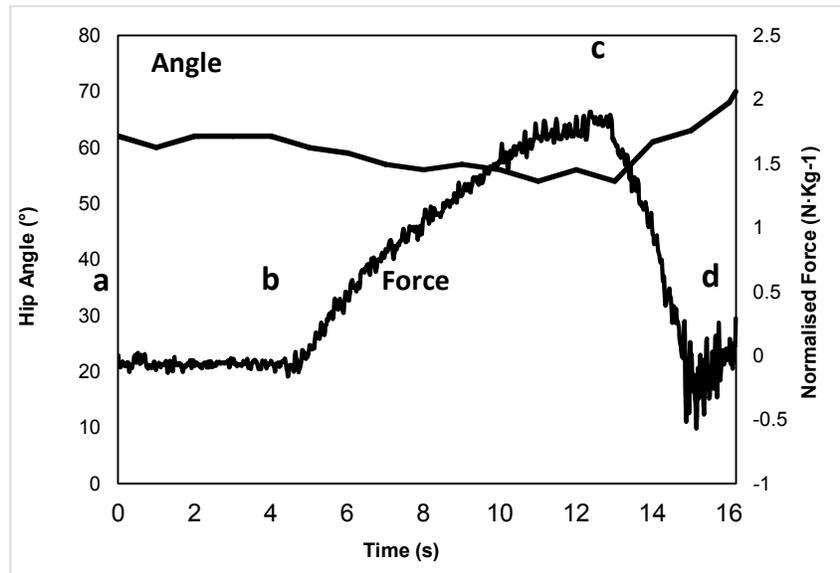


Fig. 2. DINABANG angle and force measurements

Phase a-b: familiarization at most comfortable position 60°; phase b-c: increasing isometric force; point c: lumbar region about to be lifted and interruption of effort; phase c-d: relaxing limb held in place by elastic band

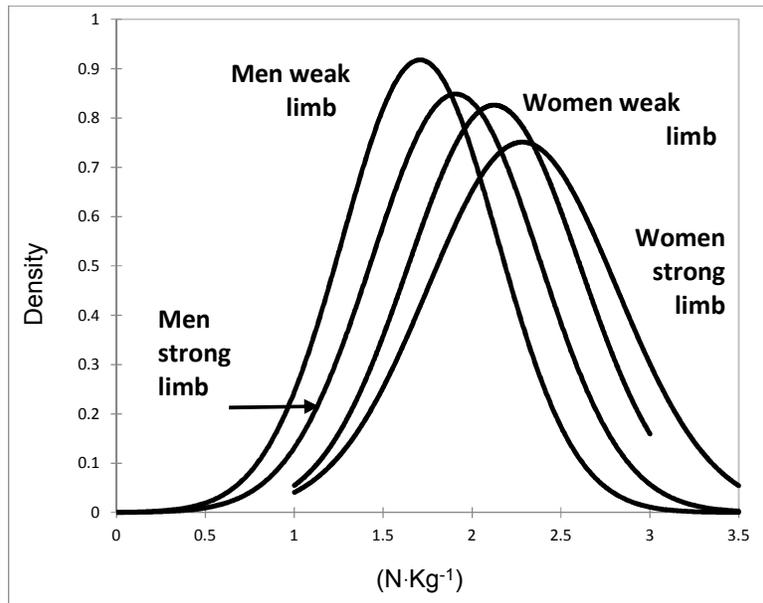


Fig. 3. Body weight adjusted normal distributions of posterior thigh isometric force
Note that the women Gaussian curve spans higher weight specific Figures than men's curve

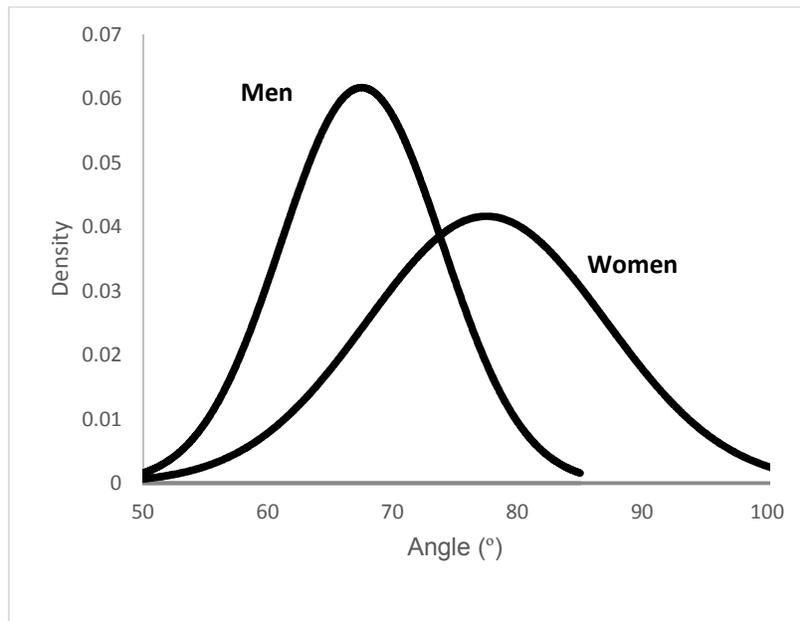


Fig. 4. Adjusted normal distributions of flexibility angles for isometric force of the lower limb
Note that the women Gaussian curve spans higher angles than men's curve by 13%

The rationale to develop DINABANG was in the first place derived from observing a significant post-operative weakness [14] of posterior hamstring muscles after Anterior Cruciate Ligament (ACL) repair after all kinds of surgical techniques. Common clinical Physical Therapy

practice was to stress mobility rehabilitation and front (quadriceps) recovery. No special attention was ever given to posterior thigh muscles. This clearly appeared to us as a limitation since no objective measurement was available to support such practices. According to our clinical

experience it is good to include strengthening of both posterior and anterior limb muscles. Posterior thigh strengthening is an important goal to work towards to, contrary to common practice which only stresses mobility and front recovery (quadriceps training). Our experience with ACL rehabilitation suggests [14] that posterior knee structures are affected by surgery of the hamstring tendon autograph because of its reduced activity [15] secondary to postsurgical pain. Therefore, one of the major problems addressed by the Physical Therapist, in addition to the rehabilitation of the functional quadriceps which is the visible aspect, is to return full functionality to the hamstring. Patients with a hamstring weakness should work towards recovery of its strength and, by doing so, inevitably face rupture risks. Until now there was nothing but clinical judgment by the Physical Therapist to control such efforts and therefore to avoid iatrogenic consequences of excess exercise. DINABANG was conceived [10] to address this very critical point of rehabilitation. It allows setting safety alarms during rehabilitation exercises. Hence, the original measurements given here for the first time are a contribution to include safety standards to limit efforts during rehabilitation. Such limits are also useful on the lower side of the normal interval, because they allow the Physical Therapist to detect insufficient patient effort to fulfill the muscular strengthening goals.

Askling and Thorstensson [7] published an empirical test with unfortunately no quantitative angle measurements. We addressed this limitation by developing DINABANG instrument and by publishing the measurements we are reporting in the present paper. The use of DINABANG may in the future be useful to measure athletes' efforts during Askling's h-test as a very much-needed objective quantification. The simple maneuvers associated with DINABANG make of it a good candidate for ecological rehabilitation since it can be used in the sports field, indoor gymnasium or even the athlete's home.

The force exerted by the volunteers may appear to be of a low value. Indeed, the forces would be a lot larger in case the body was tied to the medical Table or mat. In our case, the peak force is the consequence of interrupting the increasing isometric effort when it is barely capable of lifting the body. The standard evaluation technique described in this paper and tested for the first time at the *Congreso DePunta* in 2018 is a

simple and repeatable measurement to be used in clinical settings. The objective and unmistakable situation of the lumbar region lifting from the mat is part of the protocol to measure, in a standardized way, the force exerted during this test. Since the definition of the peak force is given by the lifting of the athlete's body, we have adopted a specific unit such as $N \cdot Kg^{-1}$: heavier bodies are usually associated with higher muscle masses, thus justifying our unit selection.

DINABANG is a novel instrument now available for lower limb muscle rehabilitation. Despite the costly instrumentation offered on the market for isokinetic and isometric evaluation, DINABANG only uses simple and common elements such as an elastic band, a strap around the distal tibia, a microcontroller/Bluetooth® device and a laptop computer. This outfit is readily available in the outpatient unit or in the training field. Normal values of body weight specific effort are available after the 74 measurements published in the present paper which will be included in the DINABANG software. The use of such an instrument for bilateral evaluation over time will allow monitoring the rehabilitation progression and may be used to detect any limb asymmetry. The contribution of this research may in the near future have consequences on the efficiency of elite athletes training and on their performance.

5. CONCLUSION

DINABANG is a novel clinical instrument which needed normal values to be included as real time alarms during rehabilitation exercises. The measurements of body-mass-normalised peak forces and of the flexibility angle reported here fill this need and, at the same time, constitute unpublished normal measurements for young healthy adults. DINABANG for the first time allows to perform safely a motor task within the medical office in very much the same way it is done in the sports field. It can be said that DINABANG is compatible with an ecological approach to rehabilitation. The inherent safety of DINABANG is due to its capacity to measure efforts and to alert of any excess.

CONSENT

All authors declare that written informed consent was obtained from the professional and amateur sportsperson for publication of this research paper and accompanying images. A copy of the

written consent is available for review by the Editorial office/Chief Editor/Editorial Board members of this journal.

ETHICAL APPROVAL

The *Programa de Apoyo a la Investigación Estudiantil PAIE 2018* research was carried out in accordance with the guidelines contained in the declaration of Helsinki and all participants signed an informed consent approved by the University Ethics Committee of the *Hospital de Clínicas* directed by Prof. Dr. Raúl Ruggia.

ACKNOWLEDGEMENTS

The authors thank the help received from the intellectual property unit (UPI) of the Universidad de la República, Uruguay, to describe and protect all DINABANG academic findings. Thanks, are given to Physical Therapists Nicoll López and Andrés Rey who were responsible for the organization of the DINABANG measurements setting at *Congreso de Punta*. The authors also acknowledge the tutorship of three electronics engineering student authors by Dr. Pablo Pérez and Dr. Francisco Veirano. The authors also thank Prof. Dr. Fernando Silveira for general guidance and support since the beginning of the DINABANG project. A special acknowledgement is here expressed to Dr. Edgardo Barboza (AUF-Uruguay National Football Team Medical Officer) for useful comments and motivation as well as to *Maestro Oscar Washington Tabares*, (AUF-Uruguay National Football Team Coach). Special thanks are expressed here to Dr. Valentina Agostini who made very useful comments and suggestions on previous versions of this paper.

COMPETING INTERESTS

Authors have declared that no competing interests exist.

REFERENCES

1. Monajati A, Larumbe-Zabala E, Goss-Sampson M, Naclerio F. Analysis of the hamstring muscle activation during two injury prevention exercises. *J Hum Kinet.* 2017;60(1):29–37.
2. Erickson LN, Sherry MA. Rehabilitation and return to sport after hamstring strain injury. *J Sport Heal Sci.* 2017;6(3):262–70.
3. Dos Santos T, Thomas C, Comfort P, McMahon, Jones P. Relationships between isometric force-time characteristics and dynamic performance. *Sports.* 2017;5(3):68.
4. Wan X, Qu F, Garrett WE, Liu H, Yu B. The effect of hamstring flexibility on peak hamstring muscle strain in sprinting. *J Sport Heal Sci.* 2017;6(3):283–9.
5. Schache AG, Wrigley TV, Baker R, Pandy MG. Biomechanical response to hamstring muscle strain injury. *Gait Posture.* 2009; 29(2):332–8.
6. Ramos GA, Arliani GG, Astur DC, Pochini A de C, Ejnisman B, Cohen M. Rehabilitation of hamstring muscle injuries: a literature review. *Rev Bras Ortop (English Ed [Internet].* 2017;52(1):11–6. Available:https://linkinghub.elsevier.com/retrieve/pii/S2255497116301318
7. Askling C, Thorstensson A. Hamstring muscle strain in sprinters. *New Stud Athl.* 2008;23(3):67–79.
8. Simini F, Santos D. Anterior Cruciate Ligament reconstruction follow-up instrumentation based on Centre of Rotation videofluoroscopy determination: Development of an original equipment, CINARTRO, and first clinical use. In: Conference Record - IEEE Instrumentation and Measurement Technology Conference. 2014;923–6.
9. Ledesma MR, Braidot A, Santos D, Simini F. 3D reconstruction of knee motion by videofluoroscopy & videography with orthogonal cameras. In: XV International Symposium on 3D Analysis of Human (3DAHMM-2018); 2018. In: press.
10. Santos D, Fernández A, Barboza R, Dominguez J, Veirano F, Pérez P, et al. DINABANG: Explosive force hamstring rehabilitation biomechanics instrument. 6th Int Conf Biotechnol Bioeng 2017 Offenburg, Ger. 2017;23(1).
11. Andersen JC. Flexibility in performance: Foundational concepts and practical issues. *Athl Ther Today.* 2006;11(3):9–12.
12. Blackburn JT, Norcross MF, Padua DA. Influences of hamstring stiffness and strength on anterior knee joint stability. *Clin Biomech (Bristol, Avon).* 2011;26(3):278–83.
13. Knezevic O, Mirkov D, Marko K, Milovanovic D, Jaric S. Evaluation of isokinetic and isometric strength measures for monitoring muscle function recovery after anterior cruciate ligament reconstruction. *J Strength Cond Res.* 2014;1722–31.

14. Santos D, Massa F, Simini F. Evaluation of anterior cruciate ligament reconstructed patients should include both self-evaluation and anteroposterior joint movement estimation? *Phys Ther Rehabil.* 2015; 2(1):3.
15. Grinsven S Van, Cingel REH Van, Holla CJM, Loon CJM Van. Evidence-based rehabilitation following anterior cruciate ligament reconstruction. *Knee Surg Sport Traumatol Arthrosc.* 2010;18:1128–44.

© 2019 Santos et al.; This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Peer-review history:
The peer review history for this paper can be accessed here:
<http://www.sdiarticle3.com/review-history/49921>